

## Manual

# MagnifiQ™ Pathogen reagent and consumables kit

A set of reagents and all necessary consumables for filling plates for the automated, magnetic isolation of DNA and RNA of pathogenic microorganisms.

catalog #	size	compatible devices *
606D-16U-64	64 isolations	Auto-Pure 32A
606D-16V-64	64 isolations	Auto-Pure Mini
606D-16U-256	256 isolations	Auto-Pure 32A
606D-16V-256	256 isolations	Auto-Pure Mini
606D-96V-960	960 isolations	Auto-Pure 96

### \* Compatible devices

The kit has been tested with ThermoFisher Scientific KingFisher Flex and specific Allsheng brand isolation devices. This does not preclude it from working with other devices. If your device is not listed, please contact us at [info@aabiot.com](mailto:info@aabiot.com).

For research use only.

### Guarantee

A&A Biotechnology provides a guarantee on this product.

The company does not guarantee the correct performance of this kit in the event of:

- not adhering to the supplied protocol
- use of not recommended equipment or materials
- use of other reagents than recommended or which are not a component of the product
- use of expired or improperly stored product or its components



# Table of Contents

<b>Advantages</b>	<b>3</b>
<b>Sample types</b>	<b>3</b>
<b>Specification</b>	<b>3</b>
<b>Description</b>	<b>3</b>
<b>Contents</b>	<b>4</b>
Reagents	4
Plastic consumables	4
<b>Additional equipment and reagents</b>	<b>5</b>
Necessary	5
Optional	5
<b>Plate preparation</b>	<b>6</b>
16 samples per plate format	6
96 samples per plate format	7
<b>Material preparation</b>	<b>8</b>
1.5 ml Eppendorf tubes	8
Animal tissue	8
Blood (fresh or frozen, plasma, serum), body fluids	8
Swabs with transport medium	9
Dry swabs	9
96 deep-well plates 2.2 ml	10
Animal tissue	10
Blood (fresh or frozen, plasma, serum), body fluids	10
Swabs with transport medium	11
Dry swabs	11
<b>Protocol</b>	<b>12</b>
Protocol files	12
Extraction protocol	13
16 samples per plate format	13
96 samples per plate format	14
<b>Safety information</b>	<b>15</b>

## Advantages

- Automated, fast isolation.
- Universal extraction of both DNA and RNA Automated, fast isolation.

## Sample types

sample type	sample size
Animal tissue	up to 20 mg
Blood (fresh or frozen, plasma, serum), body fluids	up to 200 µl
Swab	1 pc

## Specification

protocol time	~ 30 min
elution volume	50 - 100 µl
elution solution	Tris buffer (10 mM, pH 8.5)
binding capacity	30 µg DNA/RNA
downstream applications	qPCR, RT-qPCR, sequencing

## Description

**MagnifiQ™ Pathogen reagents and consumables kit** is designed for RNA and DNA isolation from viruses and Gram(-) bacteria. The kit contains reagents and all necessary consumables for self-filling plates. The isolated material is perfect for further analyzes and tests by qPCR and RT-PCR methods and for sequencing.

The **MagnifiQ™** series products are based on the automated isolation of nucleic acids with use of magnetic beads. This method significantly shortens working time and reduces risk of mistake in comparison to manual methods.

# Contents

## Reagents

składnik	64 isolations		256 isolations		960 isolations		storage
	quantity	cat #	quantity	cat #	quantity	cat #	
<b>BBG binding buffer</b>	40 ml	K-BBG-40	155 ml	K-BBG-155	580 ml	K-BBG-580	15–25 °C
<b>A1WI wash solution</b>	55 ml	K-A1WI-55	225 ml	K-A1WI-225	850 ml	K-A1WI-850	15–25 °C
<b>MQBB magnetic beads</b>	45 ml	K-MQBB15-45	170 ml	K-MQBB15-170	640 ml	K-MQBB15-640	15–25 °C
<b>Tris buffer</b>	8 ml	K-TRIS-8	30 ml	K-TRIS-30	110 ml	K-TRIS-110	15–25 °C
<b>LTE 2X buffer</b>	15 ml	K-LTE2X-15	55 ml	K-LTE2X-55	210 ml	K-LTE2X-210	15–25 °C
<b>Proteinase K</b>	1,5 ml	K-PRK-15A	6 ml	K-PRK-6	22 ml	K-PRK-22	2–8 °C*

\* Proteinase K can be stored at 15–25 °C for up to 12 months.

## Plastic consumables

606D-16U-64			606D-16U-256		
component	quantity	cat #	quantity	cat #	storage
<b>2.2 ml plate</b>	4 pcs	K-P96U22	16 pcs	K-P96U22	15–25 °C
<b>tip comb 8</b>	4 x 2 pcs	K-C8U-2	16 x 2 pcs	K-C8U-2	15–25 °C
<b>protective film</b>	4 pcs	K-MQF-4	16 pcs	K-MQF-16	15–25 °C

606D-16V-64			606D-16V-256		
component	quantity	cat #	quantity	cat #	storage
<b>2.2 ml plate</b>	4 pcs	K-P96V22	16 pcs	K-P96V22	15–25 °C
<b>tip comb 8</b>	4 x 2 pcs	K-C8U-2	16 x 2 pcs	K-C8U-2	15–25 °C
<b>protective film</b>	4 pcs	K-MQF-4	16 pcs	K-MQF-16	15–25 °C

**604D-96V-960**

component	quantity	cat #	storage
CP - comb plate	1 pc	K-P96V22C	15–25 °C
2.2 ml plate	50 pcs	K-P96V22	15–25 °C
0.5 ml plate	2 x 5 pcs	K-P96V05-5	15–25 °C
tip comb 96	5 x 2 pcs	K-C96V-2	15–25 °C
protective film	10 pcs	K-MQF-10	15–25 °C

## Additional equipment and reagents

### Necessary

- automated pipette
- pipette tips
- 80% ethanol (1.6 ml per sample)


### Optional

- 2 ml sterile Eppendorf tubes (sample lysis)
- sterile water, Tris buffer, PBS buffer
- vortex

# Plate preparation

## 16 samples per plate format

Distribute the buffers into a 2.2 ml plate as shown in the diagram below:

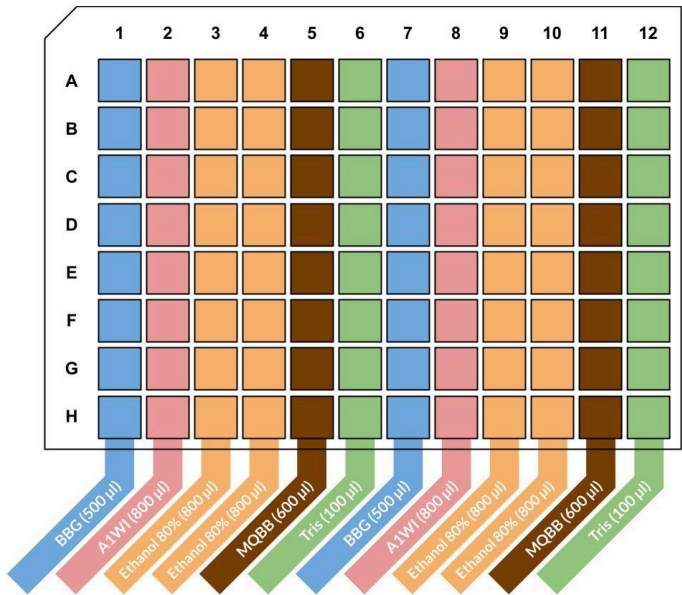

## 96 samples per plate format

Distribute the buffers into a plates and mark them as shown in the diagram below:

"SP" (2.2 ml plate)

	1	2	3	4	5	6	7	8	9	10	11	12
A												
B												
C												
D												
E												
F												
G												
H												

BBG (500 µl)

"WP 1" (2.2 ml plate)

	1	2	3	4	5	6	7	8	9	10	11	12
A												
B												
C												
D												
E												
F												
G												
H												

A1WI (800 µl)

"WP 2-3" (2.2 ml plate)

	1	2	3	4	5	6	7	8	9	10	11	12
A												
B												
C												
D												
E												
F												
G												
H												

Ethanol 80% (800 µl)

"WP 2-3" (2.2 ml plate)

	1	2	3	4	5	6	7	8	9	10	11	12
A												
B												
C												
D												
E												
F												
G												
H												

Ethanol 80% (800 µl)

"BP" (2.2 ml plate)

	1	2	3	4	5	6	7	8	9	10	11	12
A												
B												
C												
D												
E												
F												
G												
H												

MQBB (600 µl)

"EP" (0.5 ml plate)

	1	2	3	4	5	6	7	8	9	10	11	12
A												
B												
C												
D												
E												
F												
G												
H												

Tris (100 µl)

## Material preparation

### 1.5 ml Eppendorf tubes

#### Animal tissue

1. Homogenize up to **20 mg** of animal tissue in the PBS or Tris buffer.
2. Centrifuge the sample for **1 min** at **500 RPM**.
3. Transfer **200 µl** of the supernatant to 1.5 ml Eppendorf tube with lock.
4. Add **200 µl** of **LTE 2X** buffer and **20 µl** of **Proteinase K**.
5. Vortex the sample for **10 s**.
6. Follow point 1. of the [Extraction Protocol](#).

#### Blood (fresh or frozen, plasma, serum), body fluids

1. Transfer **200 µl** of the sample to 1.5 ml Eppendorf tube with lock.
2. Add **200 µl** of **LTE 2X** and **20 µl** **Proteinase K**.
3. Vortex the sample for **10 s** and incubate for **10 min** at **50 °C** with shaking.  
**Note.** If automatic shaking is not available, mix the samples by inverting the tubes a few times.
4. Centrifuge for **20 s** at **10 000 RPM**.
5. **Attention.** In the Extraction Protocol, use the supernatant as the sample.  
Follow point 1. of the [Extraction Protocol](#).



## Swabs with transport medium

No additional material preparation is required.

- 1 Follow point 1. of the [Extraction Protocol](#).

## Dry swabs

1. Break or cut off part of the swab with the collected sample and place it in 1.5 ml Eppendorf tube with lock.

**Note.** The portion of the swab with the collected sample should fit completely into the tube.

2. Add **500 µl** of sterile water, **Tris** buffer or **PBS** buffer.

**Note.** Part of the swab with the sample should be completely immersed in the buffer.

3. Leave at room temperature for **10 min**.

4. Vortex for **10 s**.

5. Transfer **200 µl** of supernatant to new 1.5 ml Eppendorf tube with lock.

6. Add **200 µl** of **LTE 2X** buffer and **20 µl** of **Proteinase K**.

7. Follow point 1. of the [Extraction Protocol](#).

## 96 deep-well plates 2.2 ml

### Animal tissue

1. Homogenize up to **20 mg** of animal tissue in the PBS or Tris buffer.
2. Centrifuge the sample for **1 min** at **500 RPM**.
3. Transfer **200 µl** of the supernatant to the well of the 96 deep-well plate (not included).
4. Add **200 µl** of **LTE 2X** buffer and **20 µl** of **Proteinase K**.  
Mix the contents of the wells by pipetting.
5. Follow point 1. of the [Extraction Protocol](#).

### Blood (fresh or frozen, plasma, serum), body fluids

1. Transfer **200 µl** the sample to the 96 deep-well plate (not included).
2. Add **200 µl** of **LTE 2X** and **20 µl** of **Proteinase K** to the wells.  
Mix the contents of the wells by pipetting.
3. Seal the plate with a protective film and incubate for **20 min** at **55 °C** with mixing **1600 RPM**.
4. Centrifuge for **1 min** at **1000 x g**.
5. **Attention.** In the Extraction Protocol, use the supernatant as the sample.  
Follow point 1. of the [Extraction Protocol](#).

## Swabs with transport medium

No additional material preparation is required.




- 1 Follow point 1. of the [Extraction Protocol](#).

## Dry swabs

1. Break or cut off part of the swab with the collected sample and place it in the wells of 96 deep-well plate (not included).
2. Add **500 µl** of sterile water, **Tris** buffer or PBS buffer.  
**Note.** Part of the swab with the sample should be completely immersed in the buffer.
3. Leave at room temperature for **10 min**.
4. Mix the contents of the wells by pipetting.
5. Transfer **200 µl** of supernatant to the new 96 deep-well plate (not included).
6. Add **200 µl** of **LTE 2X** buffer and **20 µl** of **Proteinase K**.
7. Follow point 1. of the [Extraction Protocol](#).

# Protocol

## Protocol files


device	protocol name	protocol file	installation
Auto-Pure Mini	MQ-UNI-MI	<a href="http://aabiotech.com/protocols/magnifiq/MI/MQ-UNI-MI.txt">aabiotech.com/protocols/magnifiq/MI/MQ-UNI-MI.txt</a>	<ol style="list-style-type: none"> <li>1. Create folder "items" on a USB drive and copy the protocol file to it.</li> <li>2. Insert the USB drive into a USB slot in the device.</li> <li>3. On a device screen, go to Settings &gt; System &gt; Transfer &gt; Import.</li> <li>4. Select the protocol and tap "Import".</li> </ol>
Auto-Pure Mini (QR code)	MQ-UNI-MI		<ol style="list-style-type: none"> <li>1. On a device screen, go to Run &gt;  &gt; </li> <li>2. Scan the QR code with the device's scanner.</li> </ol>
Auto-Pure 32A	MQ-UNI-32A	<a href="http://aabiotech.com/protocols/magnifiq/32A/MQ-UNI-32A.txt">aabiotech.com/protocols/magnifiq/32A/MQ-UNI-32A.txt</a>	<ol style="list-style-type: none"> <li>1. Create folder "items" on a USB drive and copy the protocol file to it.</li> <li>2. Insert the USB drive into a USB slot in the device.</li> <li>3. On a device screen, go to Settings &gt; Im.&amp;Export &gt; Import.</li> <li>4. Select the protocol and tap "Import."</li> </ol>
Auto-Pure S32	MQ_UNI_S32	<a href="http://aabiotech.com/protocols/magnifiq/S32/MQ_UNI_S32.txt">aabiotech.com/protocols/magnifiq/S32/MQ_UNI_S32.txt</a>	<ol style="list-style-type: none"> <li>1. Create folder "im_export_protocols" on a USB drive and copy the protocol file to it.</li> <li>2. Insert the USB drive into a USB slot in the device.</li> <li>3. On a device screen, go to Protocols &gt; Import.</li> <li>4. Select the protocol and tap "Import".</li> </ol>
Auto-Pure 96	MQ-UNI-96	<a href="http://aabiotech.com/protocols/magnifiq/96/MQ-UNI-96.txt">aabiotech.com/protocols/magnifiq/96/MQ-UNI-96.txt</a>	<ol style="list-style-type: none"> <li>1. Create folder "items" on a USB drive and copy the protocol file to it.</li> <li>2. Insert the USB drive into a USB slot in the device.</li> <li>3. On a device screen, go to Settings &gt; Im.&amp;Export &gt; Import.</li> <li>4. Select the protocol and tap "Import."</li> </ol>

## Extraction protocol

### 16 samples per plate format


1. Add **400 µl** of samples to the wells in columns **1** and **7** of **2.2 ml plate**.
2. Place one or two **2.2 ml plates** in the extraction device..
3. Place the appropriate number of **tip combs 8** in the extraction device.
4. Run the protocol on your device.
5. After the program is over, remove the combs and then remove the **2.2 ml plate** from the extraction device and seal it with **protective film**. The extracted DNA is located in columns **6** and **12**.

**Note.** For longer storage of extracted material, transfer it from the plate to appropriate tubes and store at 4 °C for DNA or -70 °C for RNA.

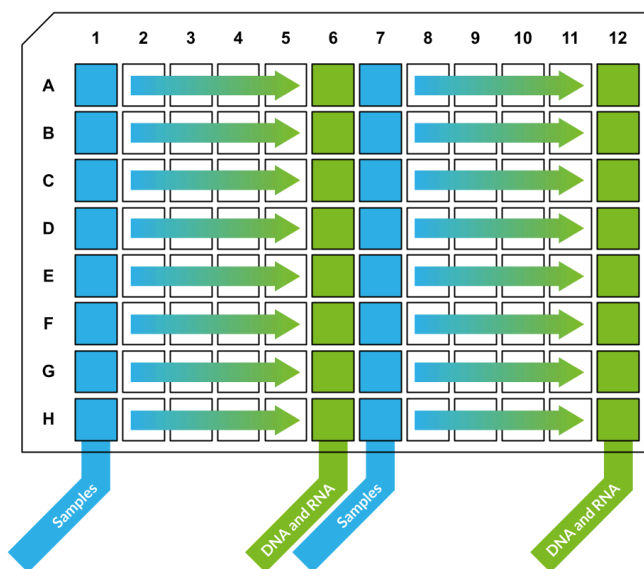

## 96 samples per plate format

1. Add **400 µl** of sample to the wells of the **SP** plate.
2. Place the **tip combs 96** into the comb plate.
3. Place the plates on the working table of the extraction device according to the diagram below:

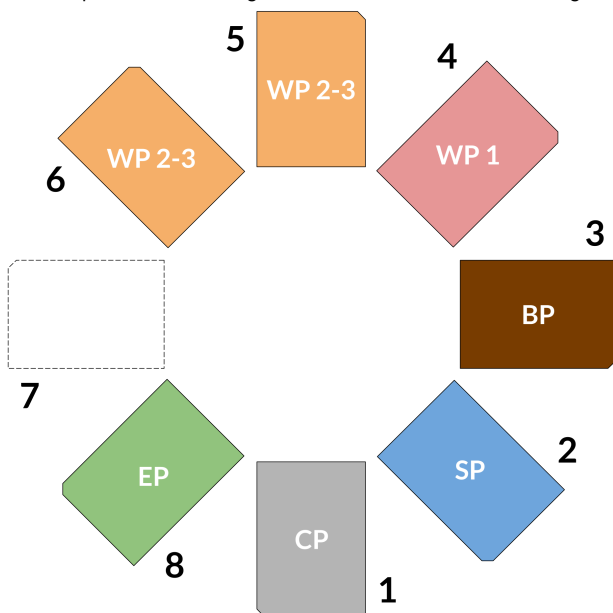

5. Run the protocol on your device.
6. After the program is over, remove the **EP** plate from the extraction device and seal it with a **protective film**.  
**Note.** For longer storage of extracted material, transfer it from the plate to appropriate tubes and store at 4 °C for DNA or -70 °C for RNA.
7. Discard remaining plates except the **CP** plate, which can be reused.

# Safety information



**DANGER**

## Proteinase K

H315 Causes skin irritation.  
 H319 Causes serious eye irritation.  
 H334 May cause allergy or asthma symptoms or breathing difficulties if inhaled.  
 H335 May cause respiratory irritation.  
 P261 Avoid breathing dust.  
 P305+P351+P338 If in eyes: rinse cautiously with water for several minutes. Remove contact lenses, if present and easy to do. Continue rinsing.  
 P342+P311 If experiencing respiratory symptoms call a Poison Center or doctor/physician.



**WARNING**

## LTE 2X

H302 Harmful if swallowed.  
 H315 Causes skin irritation.  
 H319 Causes serious eye irritation.  
 P305+P351+P338 If in eyes: rinse cautiously with water for several minutes. Remove contact lenses, if present and easy to do. Continue rinsing.



**DANGER**

## BBG binding buffer

H302+H312+H332 Harmful if swallowed, in contact with skin or if inhaled.  
 H314 Causes severe skin burns and eye damage.  
 H412 Harmful to aquatic life with long lasting effects.  
 P273 Avoid release to the environment.  
 P280 Wear protective gloves/protective clothing/eye protection/face protection/hearing protection.  
 P301+P312+P330 If swallowed: Call a poison center/doctor/... if you feel unwell.  
 P303+P361+P353 If on skin (or hair): Take off immediately all contaminated clothing. Rinse skin with water or shower.  
 P304+P340 If inhaled: Remove person to fresh air and keep comfortable for breathing.  
 P305+P351+P338 If in eyes: rinse cautiously with water for several minutes. Remove contact lenses, if present and easy to do. Continue rinsing.



**DANGER**

## A1W1 wash solution

H225 Highly flammable liquid and vapor.  
 H302 Harmful if swallowed.  
 H315 Causes skin irritation.  
 H319 Causes serious eye irritation.  
 H336 May cause drowsiness or dizziness.  
 P210 Keep away from heat, hot surfaces, sparks, open flames and other ignition sources. No smoking.  
 P261 Avoid breathing dust/fume/gas/mist/vapours/ spray.  
 P280 Wear protective gloves/protective clothing/eye protection/face protection/hearing protection.  
 P301+P312+P330 If swallowed: Call a poison center/doctor/... if you feel unwell.  
 P305+P351+P338 If in eyes: rinse cautiously with water for several minutes. Remove contact lenses, if present and easy to do. Continue rinsing.  
 P337+P313 If eye irritation persists: Get medical advice/ attention.



**A&A BIOTECHNOLOGY**  
innovating life science

A&A Biotechnology, Strzelca 40, 80-299 Gdańsk  
tel. 883 323 761, 600 776 268  
info@aabiot.com, [www.aabiot.com](http://www.aabiot.com)

version 2025-1

